

Mengshen

INSTRUCTION MANUAL

Humidity & Temperature Meter

Wet Bulb Temperature

DewPoint Temperature



TABLET OF CONTENTS

TITLE

1. INTRODUCTION
2. FEATURES
3. SPECIFICATIONS
4. PANEL DESCRIPTION
5. HUMIDITY AND AIR TEMPERATURE MEASUREMENTS
6. BATTERY REPLACEMENT

viengshe

Product Overview


This product is a professional level instrument with the integrated measurement function of the ambient temperature, humidity, dew point and wet bulb temperature; it is applicable for the temperature and humidity measurement of production workshop, factory warehouses, libraries, offices, laboratories, and the family living rooms and so on;

The products are featured by the high-precision and low-power consumption digital temperature and humidity sensors and the industrial-grade LCD display, which are characterized by the advantages of beautiful appearance, ease of use, wide measurement range, high accuracy, solid and durable structure.

Technical Specifications

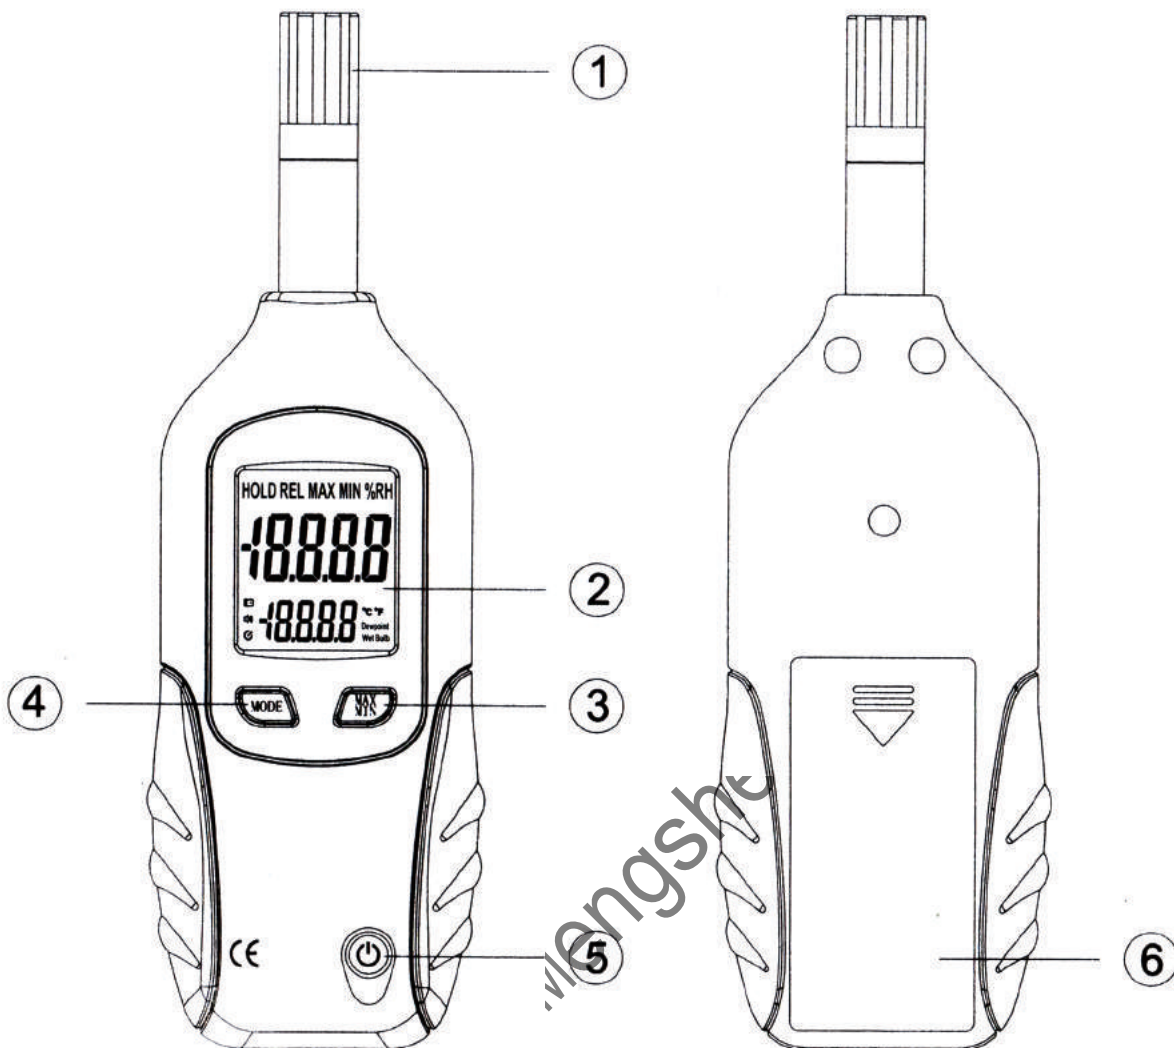
Storage environment	- 20°C ~60°C; <80%RH non-condensing
Working environment	- 20°C ~60°C
Measurement temperature range	-30°C~60°C (-22°F~140°F)
Measurement humidity range	0 ~100%RH
Dew point temperature range	- 50°C~60°C (- 58°F~140°F)
Wet bulb temperature range	- 20°C~60°C (- 4°F~140°F)
Temperature accuracy	± 0.5°C/± 0.9°F(10~55°C); ± 1.5°C/± 3°F(Other ranges)
Humidity accuracy	± 3%RH(25°C; 10%~90%RH); ± 4.5%RH (<10%或>90%RH);
Resolution	0.1%RH , 0.1°C/ , 0.1°F
Response Time	10S
Type of Battery	6F22 9V battery
Power consumption	3mA
Physical dimension	175mm x58mmx35mm
Weight	143g
Auto shutdown	≈ 15 mins

Precautions:

1. Do not put sensor in the liquid or make the sensor exposed to sunlight;
2. Do not put the instrument under extreme conditions or the heavily polluted environment such as chemical vapors, hazardous substances and so on, so as not to affect the accuracy of the meter, and even cause damage or reduce the life of the instrument;
3. Do not use solvents and detergents to clean the product, and do not disassemble the body arbitrarily for research or repair;
4. Remove the battery if do not use for a long time, so as to avoid battery leakage and corrosion of the instrument;
5. When the battery is low (LCD displays the symbol of ) , please replace the battery, so as not to affect test accuracy.

viengshe

4. PANEL DESCRIPTION



- ① **Humidity / Air Temperature Probe:** (Humidity Sensor and Semiconductor Sensor inside)
- ② **LCD display:** 4 1/2 dual digits LCD display with units of °C, °F, %RH dewpoint wet bulb and low battery "BAT" MIN /MAX HOLD, DATA HOLD indication.
- ③ **MAX/ MIN Button:**
MAX/MIN: Press MAX/MIN to enter MAX, MIN Recording mode (manual range only). Select the proper range before selecting MAX MIN to ensure that the MAX/MIN reading will not exceed the testing range. Press once to select MIN. Press again to select MAX. **Press and hold the Button for over 2 second to turn off MAX, MIN Recording.**
- ④ **°F, °C, dewpoint , wbt select Button:**
Press °F, °C, dewpoint, wbt select Button to enter select °F, °C, dewpoint, wbt Measurement
- ⑤ **Power ON/OFF Button :**
Turn the meter power ON/OFF
- ⑥ **Battery Compartment**

5. Humidity and air Temperature Measurements

1. Hold the probe in the area to be tested & allow adequate time for readings to stabilize.
2. Press °F, °C, dewpoint, WBT select Button to enter select °F, °C, dewpoint WBT Measurement.
3. Read the Relative Humidity and Air Temperature, dewpoint temperature wet bulb temperature.


NOTE: Do not immerse the probe in liquid; it is intended for use in air on.

Warning:

Don't expose the humidity sensor to direct sunlight (insolation).

Don't touch or manipulate the humidity sensor.

6. Battery Replacement

If the sign “ ” appears on the LCD display, it indicates that the battery should be replaced. Open the battery case and replace the exhausted battery with new battery. (1 x 9V battery NEDA 1604, 6F22 or equivalent)

viengshe